

FIG. 1

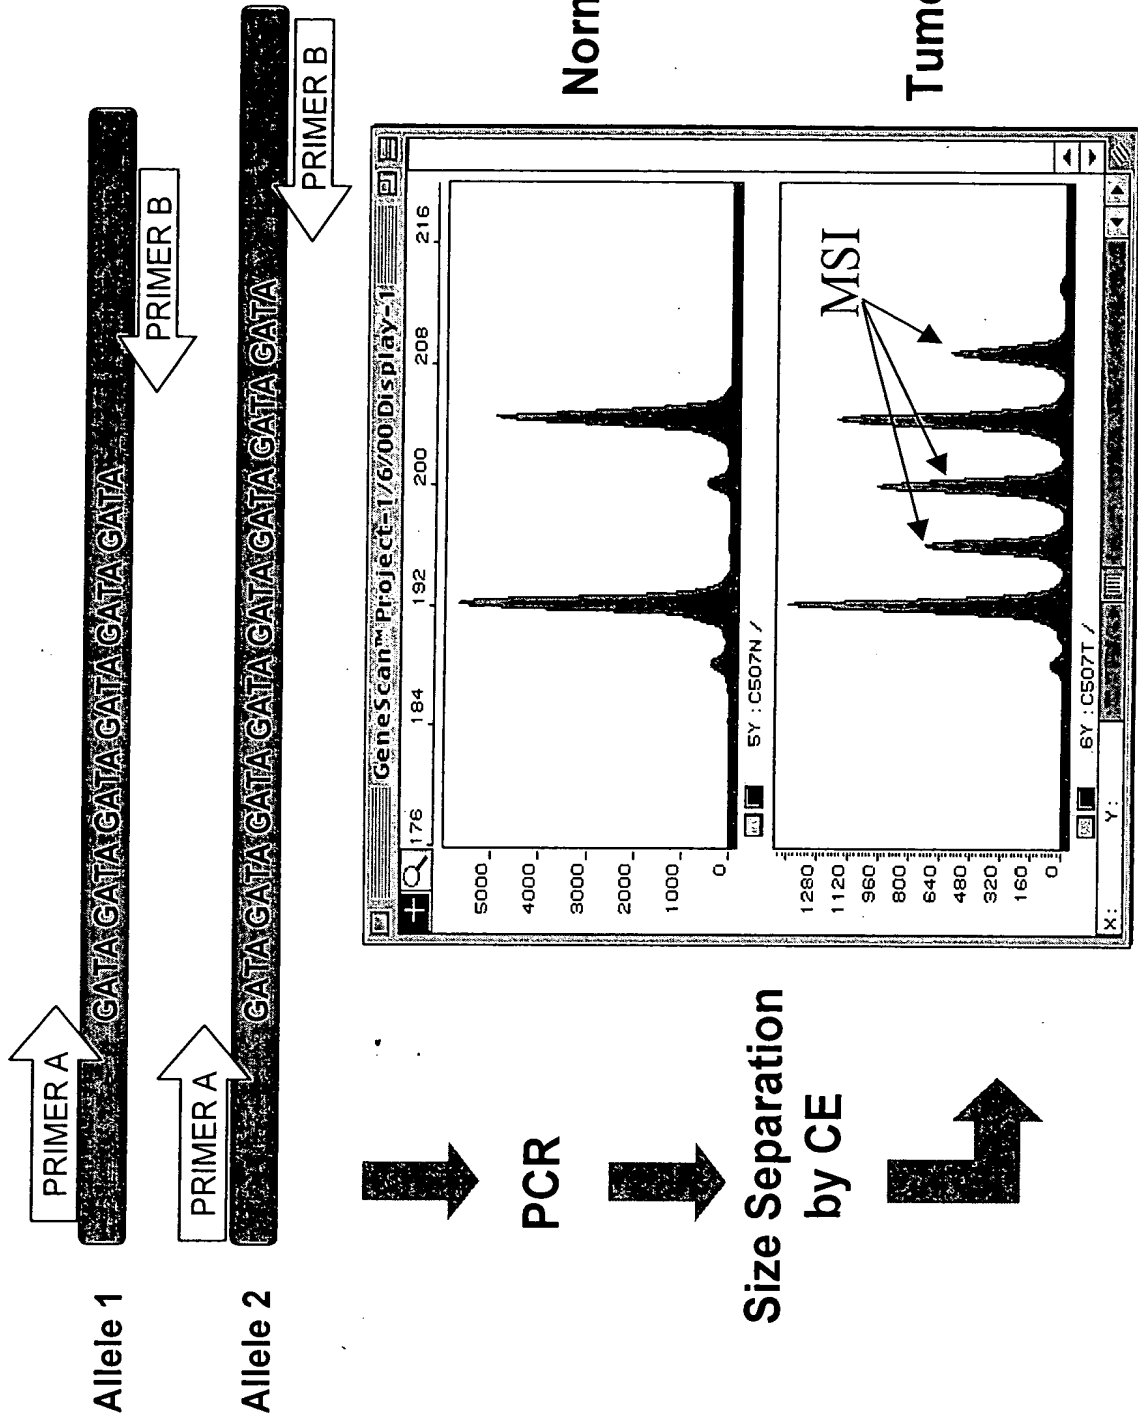
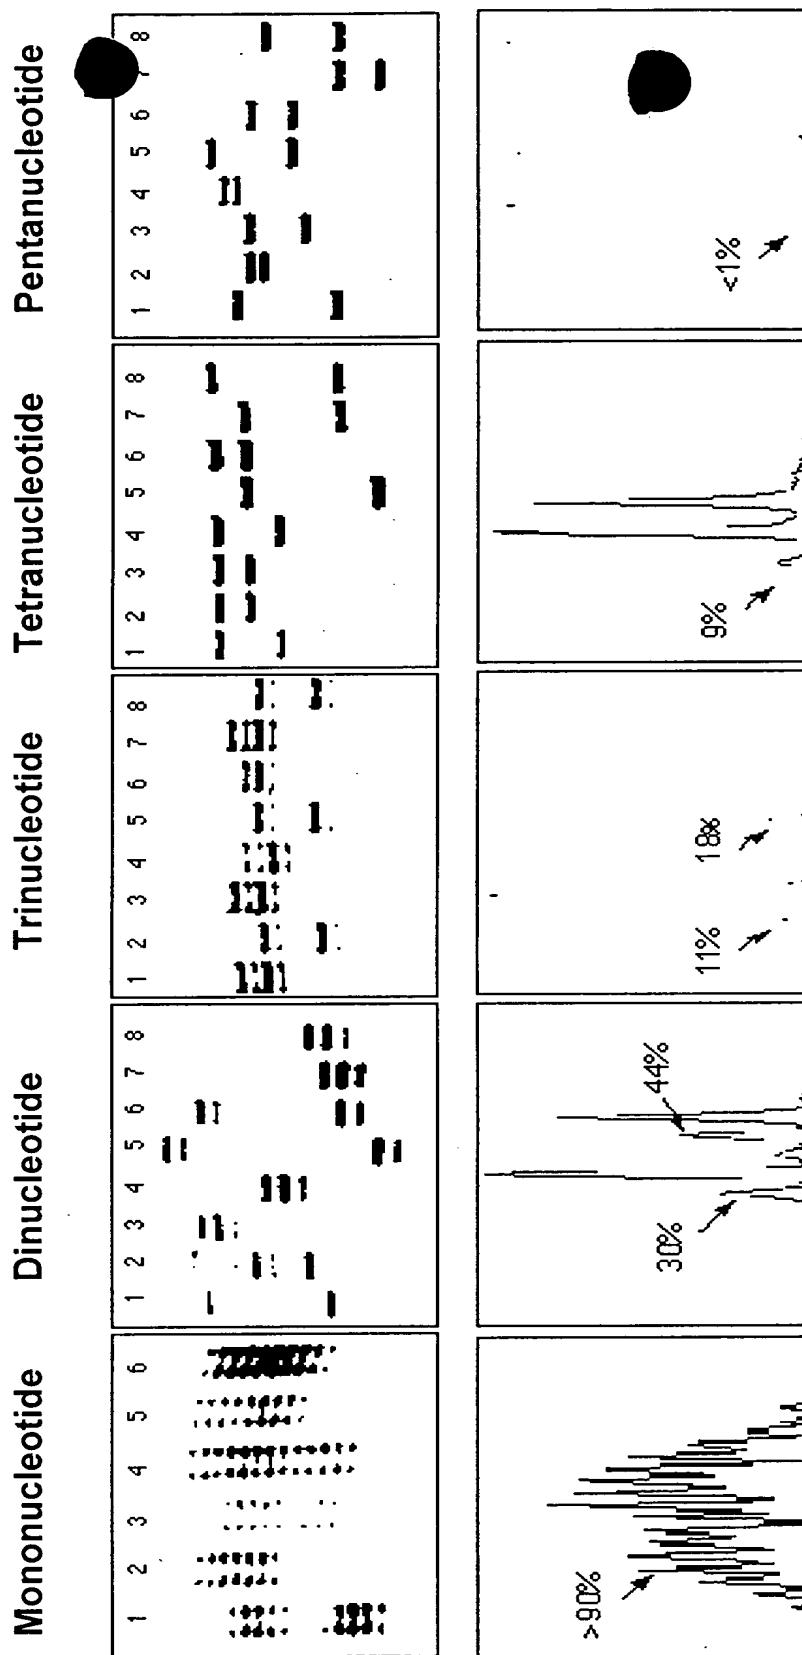


FIG. 2



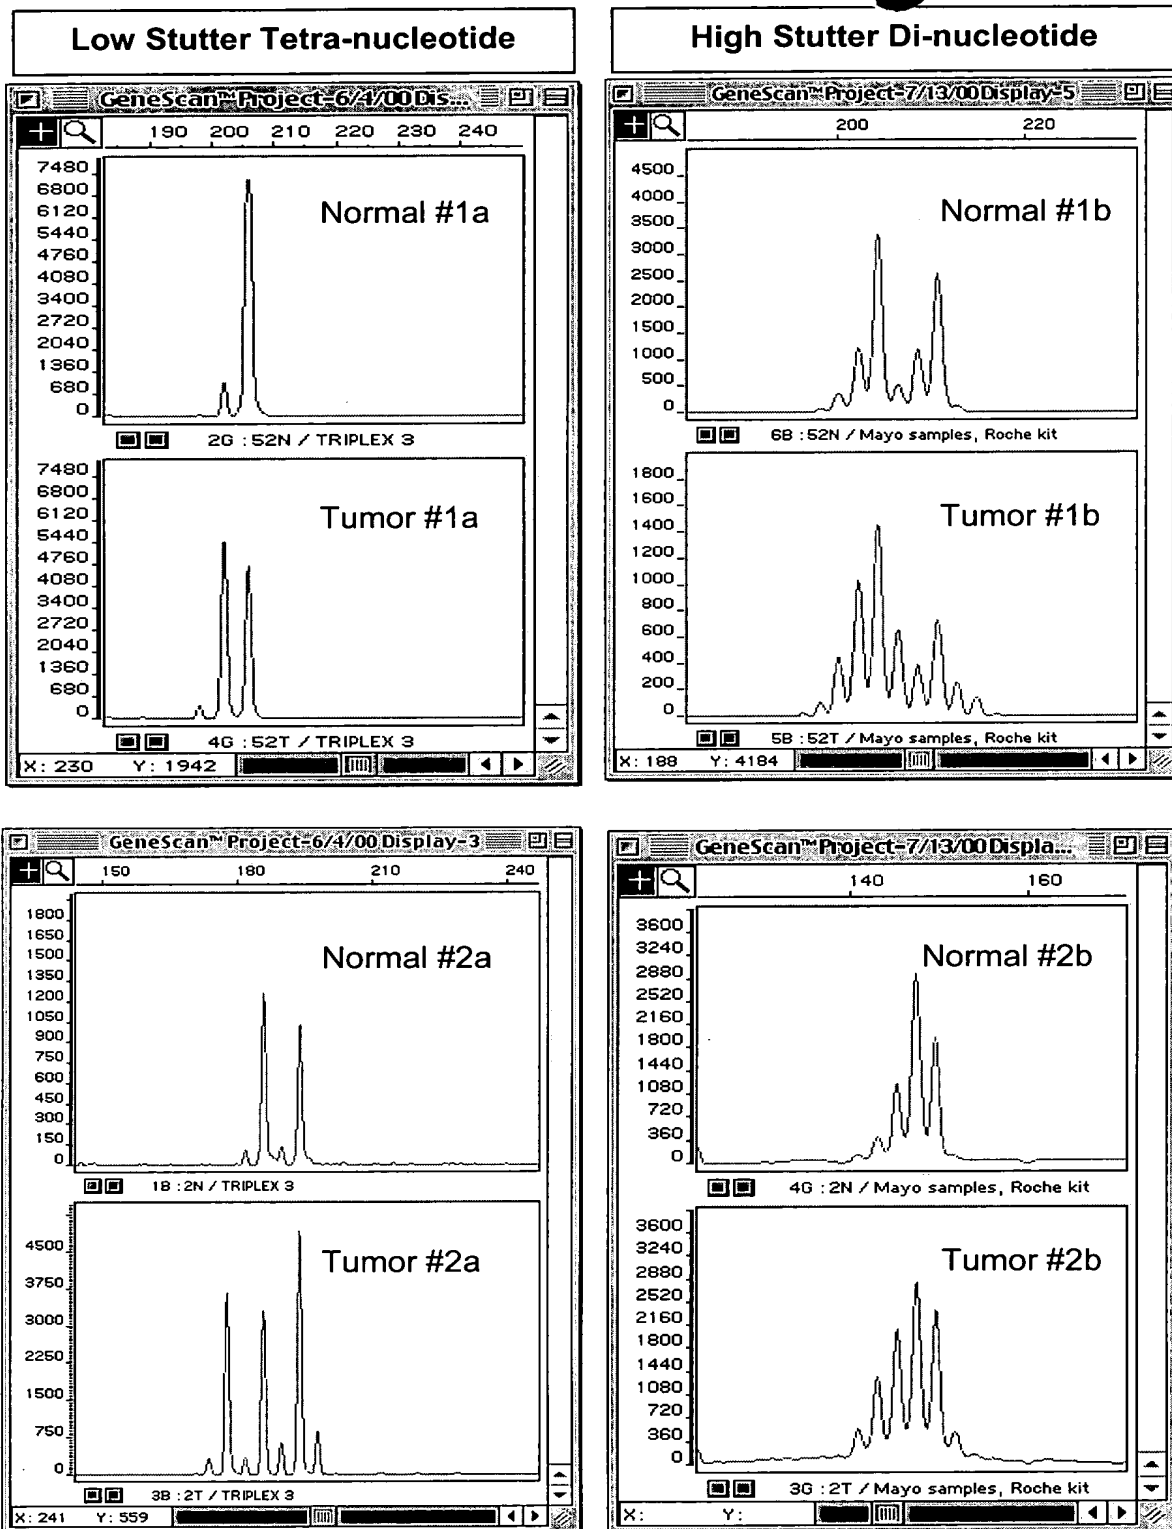


FIG. 3

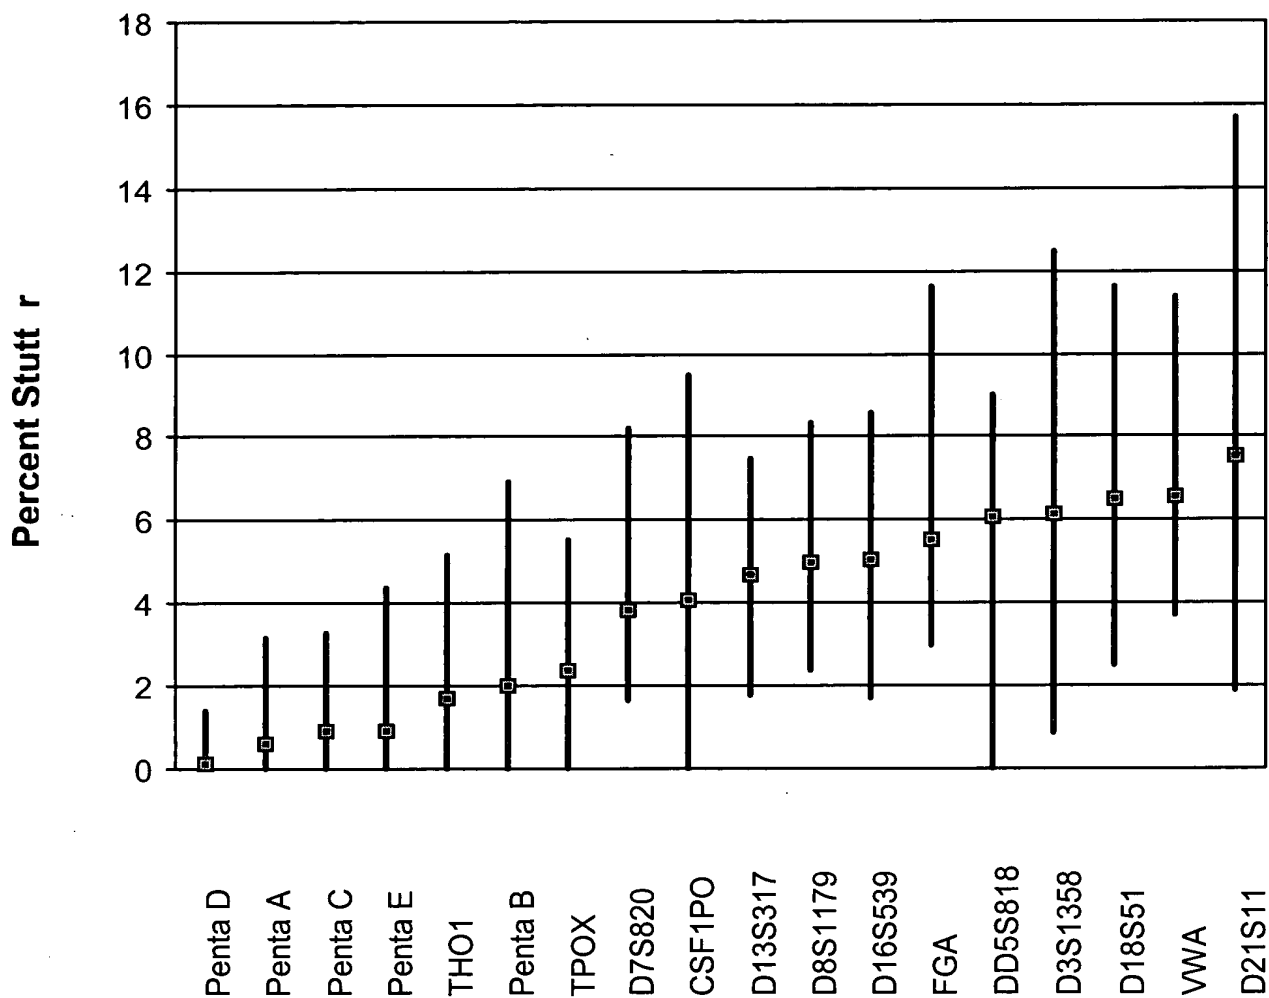


FIG. 4

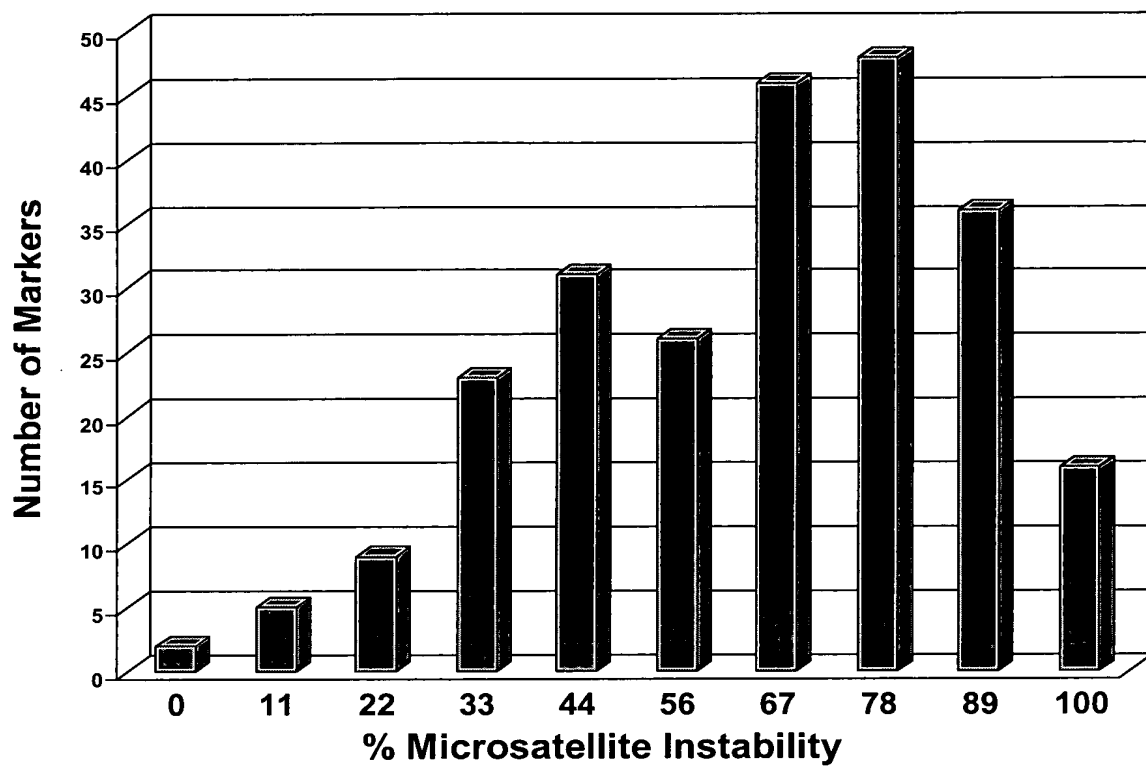


FIG. 5

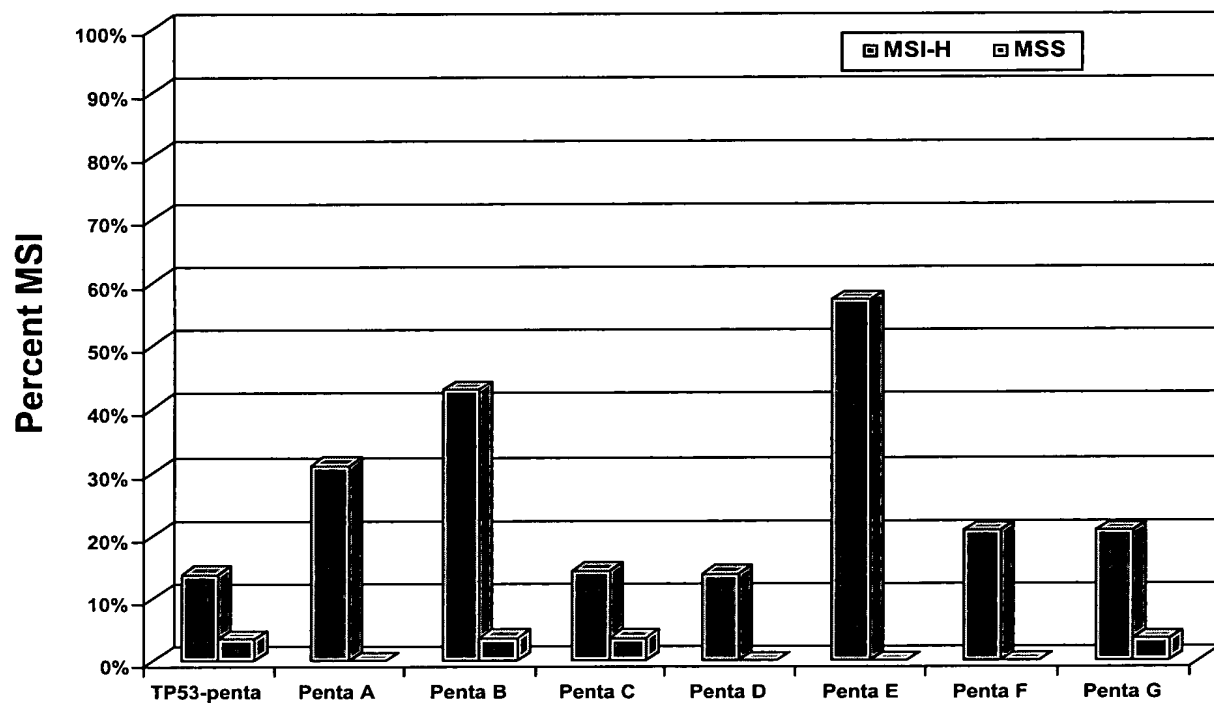


FIG. 6

FIG. 7

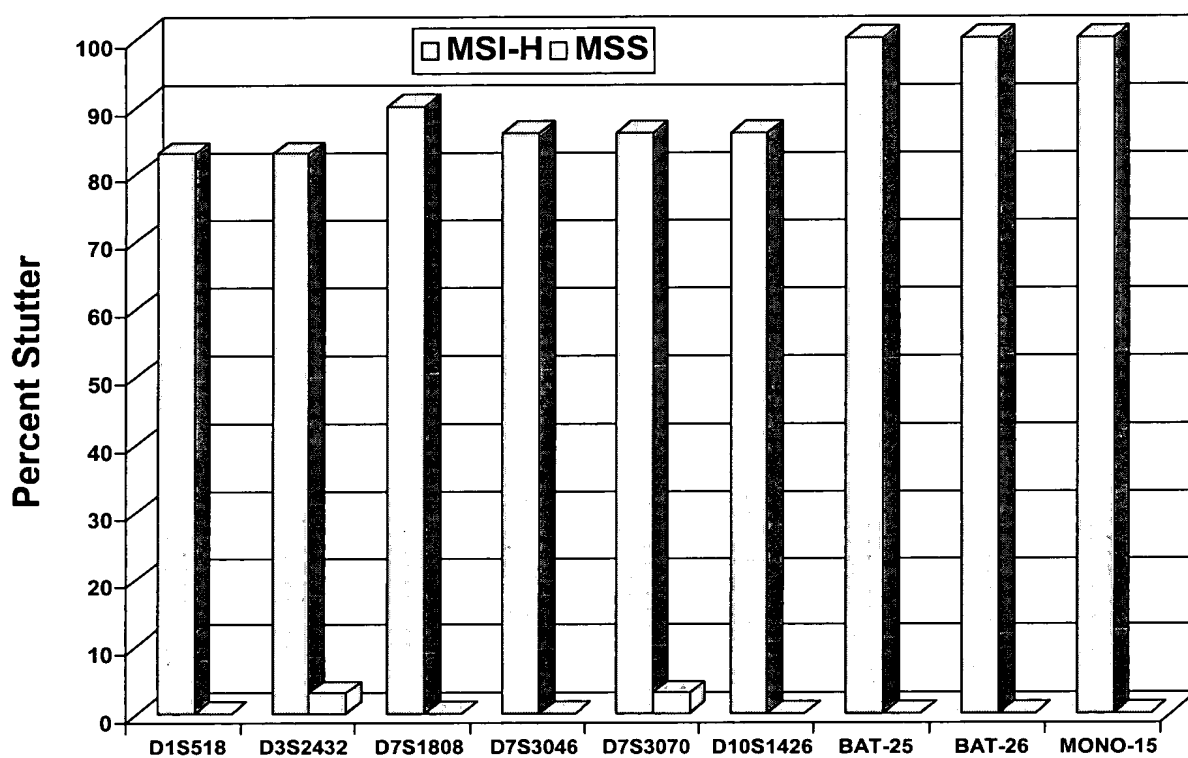


FIG. 8

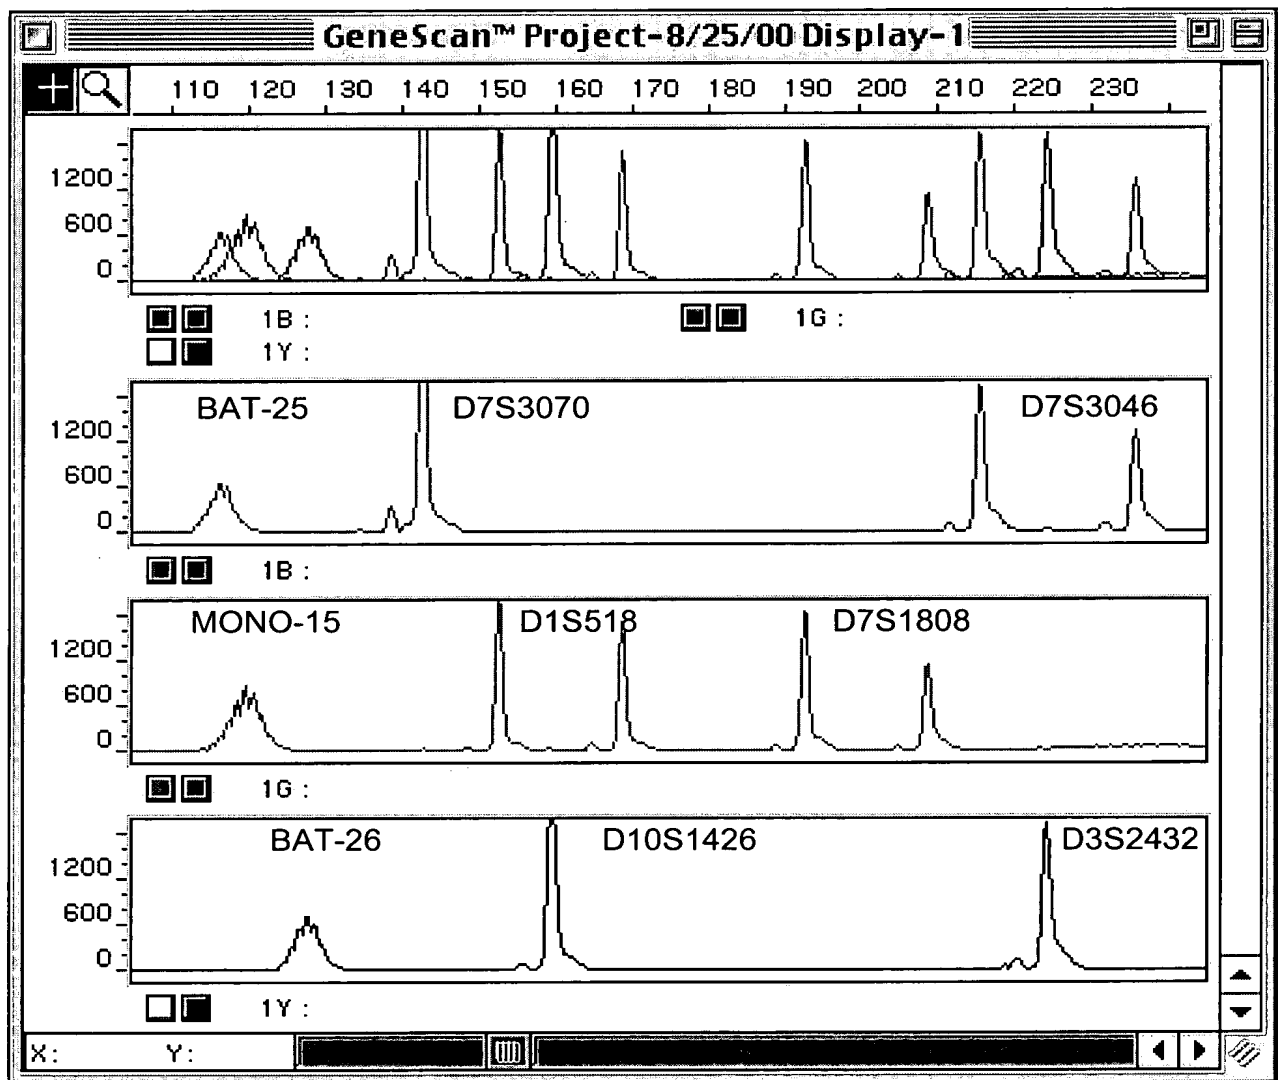


FIG. 9

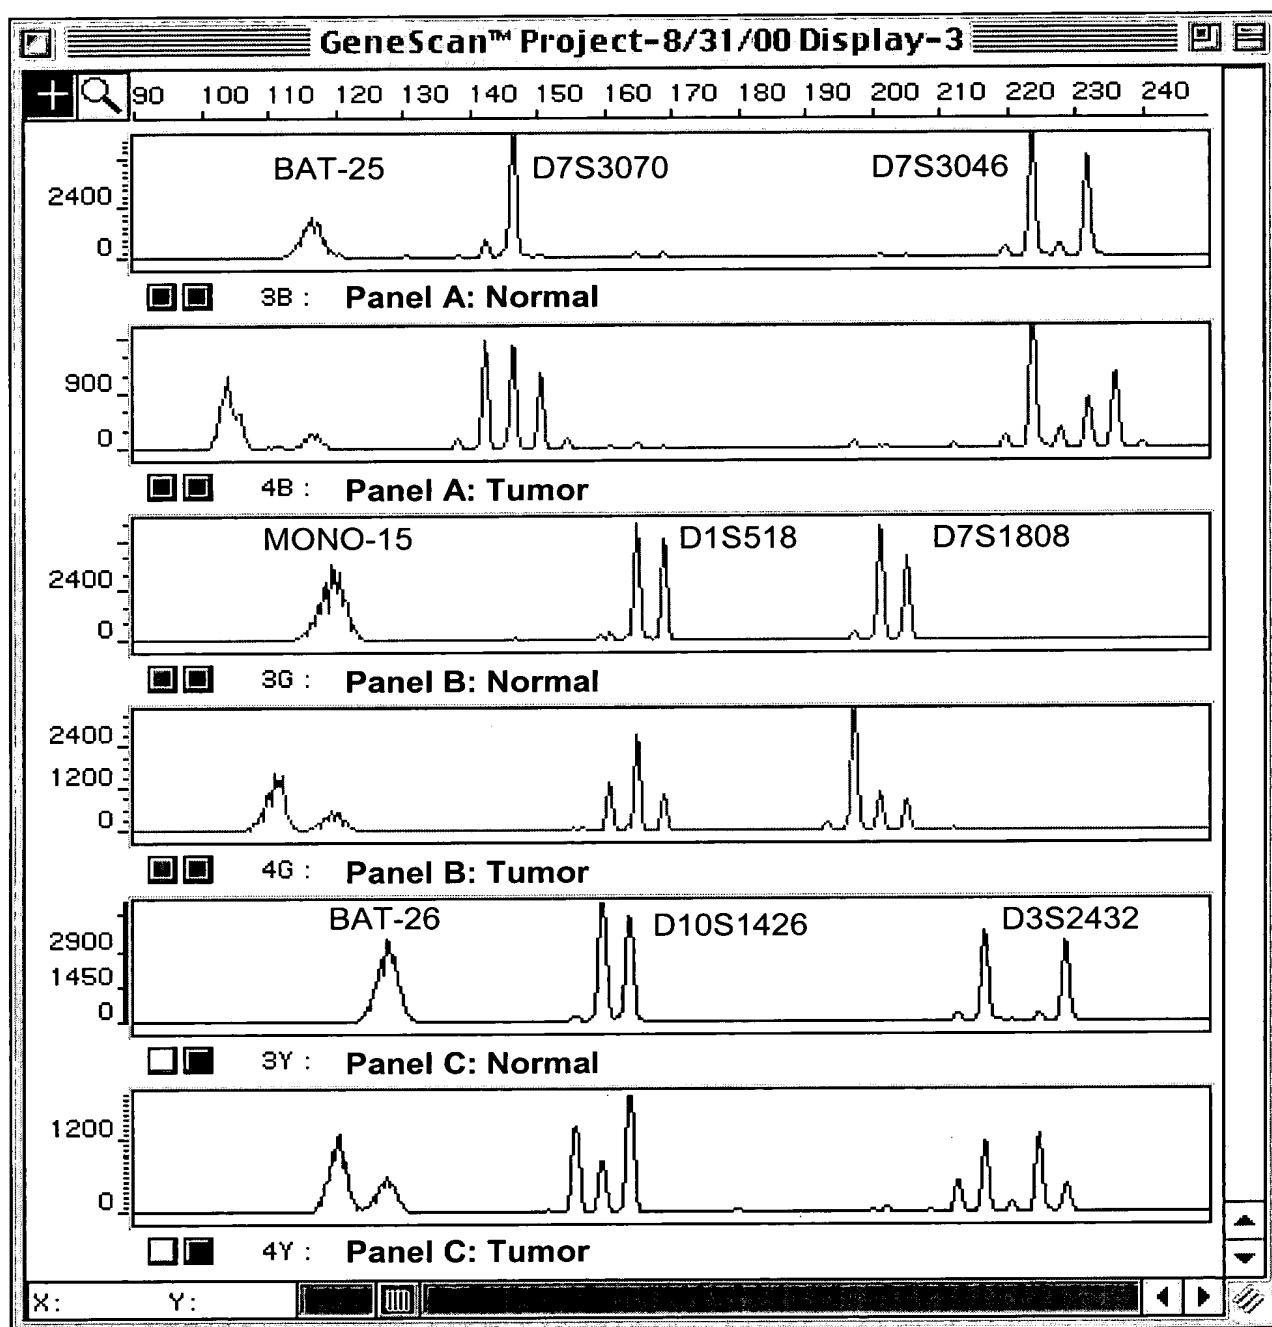


FIG. 10

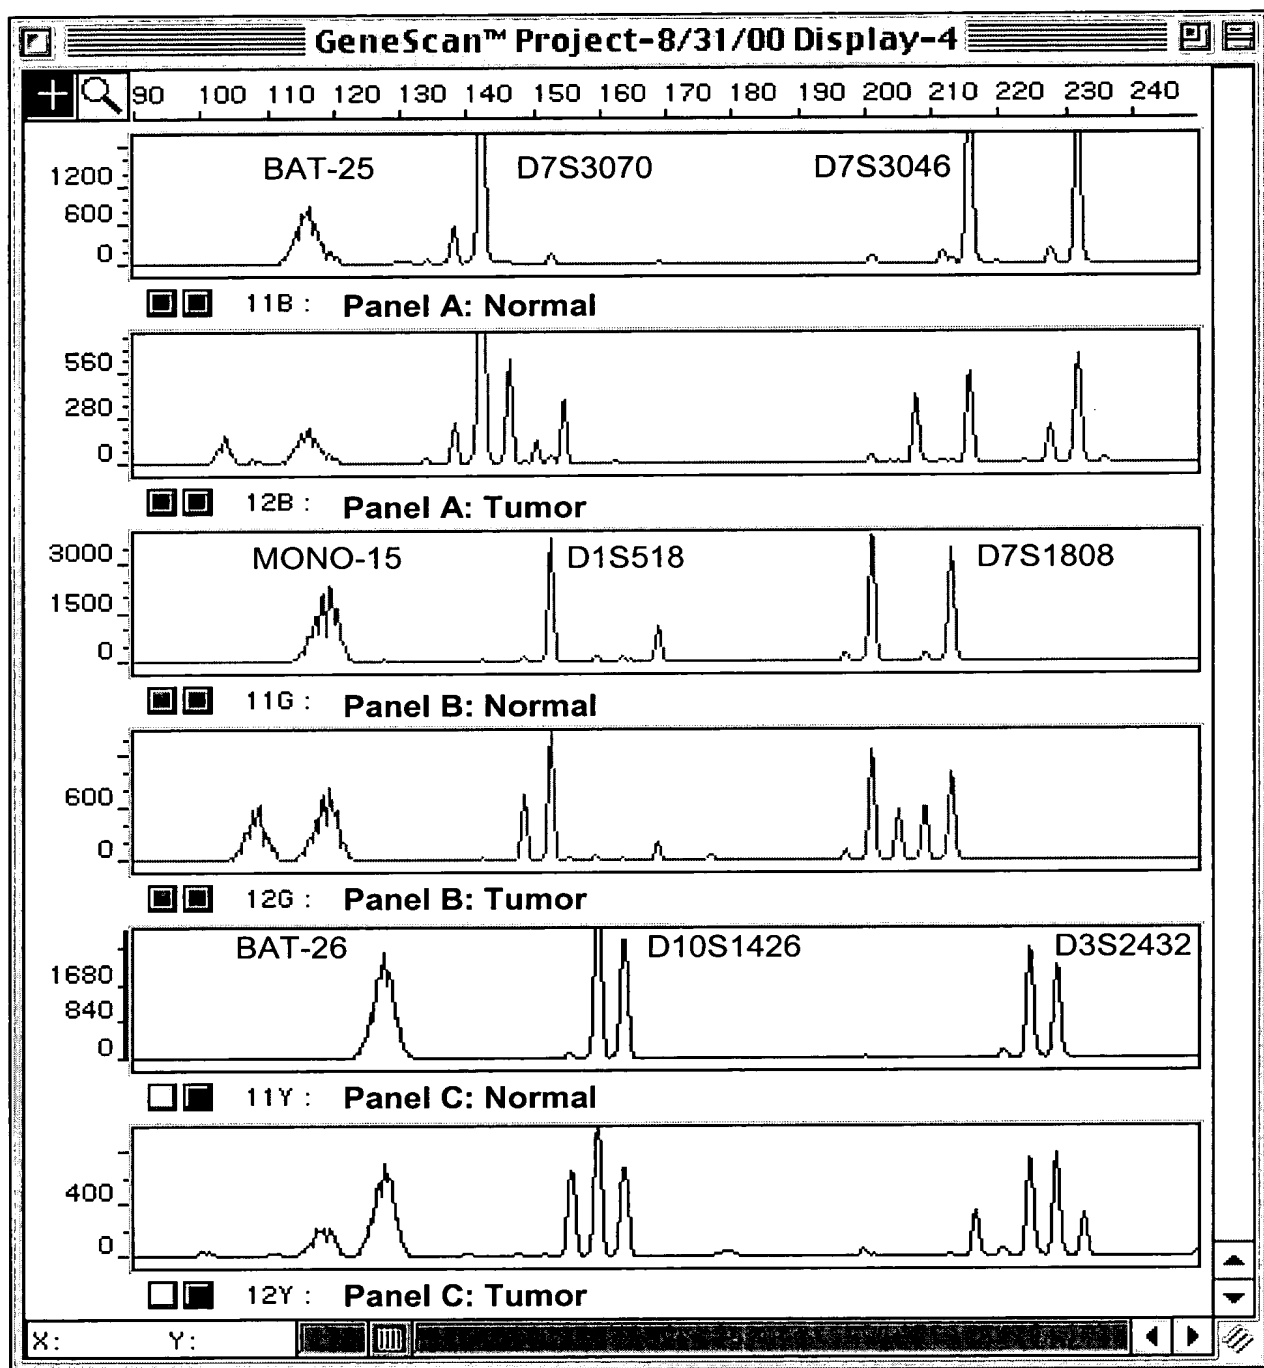


FIG. 11

GeneScan™ Project-8/31/00 Display-1

100 110 120 130 140 150 160 170 180 190 200 210 220 230

BAT-25 D7S3070 D7S3046

18B : Panel A: Normal

17B : Panel A: Tumor

MONO-15 D1S518 D7S1808

18G : Panel B: Normal

17G : Panel B: Tumor

BAT-26 D10S1426 D3S2432

18Y : Panel C: Normal

17Y : Panel C: Tumor

X: 220 Y: 317

3

GeneScan™ Project-9/1/00 Display-3

120 160 200 240

1000
500
0

2B : 2G :
2Y : 2R :

BAT-25 D7S3070 D7S3046

1000
500
0

2B : 2G :
2Y : 2R :

MONO-15 D1S518 D7S1808

1000
500
0

2B : 2G :
2Y : 2R :

BAT-26 D10S1426 D3S2432

1000
500
0

2B : 2G :
2Y : 2R :

X: 187 Y: 291

FIG. 13